


Instructions for use of Disinfection mats

1. Disinfecting mats should be placed in all passages leading to utility rooms and those where production is based on animal raw materials. In all farms entrances or establishments based on animal raw materials, additional disinfection mats should be provided.
2. In the places where the mats are used, notice boards informing about special precautions should be placed.
3. Drive-through mats should be placed in the entrances in such a way that all four wheels of the vehicle are disinfected.
4. According to the current Regulation of the Minister of Agriculture and Rural Development of February 9, 2018, the disinfecting mat used in passages between buildings, rooms and zones should be at least 100 cm long and of the width of the door. These two dimensions are important and strictly checked especially in restricted zones and virus risk areas.
5. The vehicle speed while driving through the mats must not exceed 5 km / h. Heavy vehicles must not stop, start or turn on the mats.
6. The mats should be soaked with disinfectants in accordance with the recommendations of the producers of these preparations. The solution prepared according to the instructions should be dosed in compliance with the manufacturer's guide.
7. The disinfectant should be replenished every 3-4 hours, depending on the air temperature and humidity, as well as the traffic load.
8. During soaking, it is not allowed to combine preparations of different properties and concentrations.
9. An anti-freezing agent should be added to the disinfectant used in mats remaining outside, during the winter period in freezing temperatures.
10. At temperatures lower than -10°C, the mats remaining outside should be hidden in heated rooms so that the preparation does not freeze and damage the absorbent core.
11. During heavy rainfall, non-covered mats should be hidden or covered with foil to avoid too much saturation.
12. The mat cover should be washed by hand or mechanically at a temperature of max. 60°C, the absorbent element should be rinsed in cold water.
13. The cleaned insert and cover should be dried before soaking with a disinfectant.
14. If the mat is damaged, it must be repaired or replaced with a non-defective one. In the event of a warranty claim, please refer to the warranty conditions.
15. The warranty period for drive-through disinfection mats is 6 months.

Disinfecting mat - Material specification sheet

Feature	Disinfecting mat	Drive-through mat	Non-slip mat
Spacer mesh thickness	2,30-2,50 mm	2,30-2,50 mm	2,30-2,50 mm
Spacer mesh type	100% Polyurethane	100% Polyurethane	100% Polyurethane
Spacer mesh weight	220 g/m ²	220 g/m ²	220 g/m ²
Cover material	Polyester 600/600D	Polyester 600/600D	PVC material with antislip tabs
Foam type	Polyurethane	Polyurethane	Polyurethane
Foam thickness	3 cm	4 cm	3 cm
Foam density	N1828TF	N1828TF	N1828TF
Zipper tape type	Spiral	Spiral	Spiral
Zipper tape size	5 mm	5 mm	5 mm
Zipper material	Metal	Metal	Metal

Structure of a Disinfecting mat

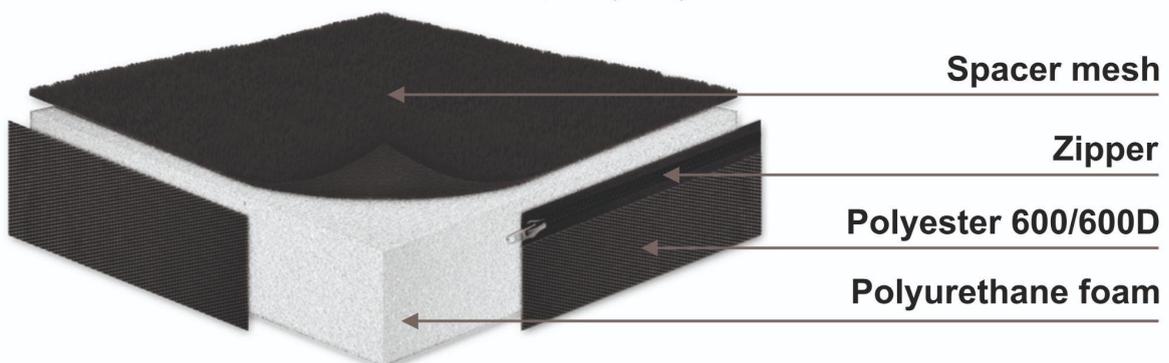


Features and description of Disinfecting mats

- The design of the mat prevents the spreading of the working liquid
- The mat has a zipper that allows the insert to be replaced
- It does not make the shoes excessively wet
- Plastic zipper tape, which will not corrode
- The mesh in the mat prevents mechanical impurities from penetrating deeply, which extends the life of the foam
- Made of strong fabrics, resistant to low temperatures
- Replaceable polyurethane foam inside of the mat
- Both the mat and its insert can be cleaned manually or mechanically

Disinfecting preparations

One of the most popular disinfectants for the mats is Virkon S by Lanxess. It is a highly effective preparation with a broad spectrum of virucidal, bactericidal, and fungicidal activity. Available in various sizes.

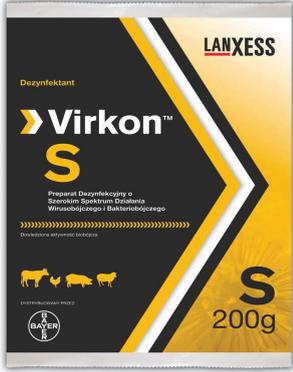10 kg package	5kg package	200g package
		

Warranty conditions for Disinfection mats

1. The warranty period for drive-through disinfection mats is 6 months.
2. Defects found during the warranty period will be removed within 3 weeks from the date of receipt of the defective goods.
3. The complaint will be considered after delivering the defective mat, proof of purchase, and completed complaint form with the defect described.
4. If the purchase document is missing and the mat was not being used following the instructions, the warranty repair will be refused.
5. The claimed mat should be delivered clean and dry.
6. The warranty covers defects resulting from flaws of the material or the manufacturer's fault, e.g. incorrectly made seams, incorrectly installed, or defective zipper.
7. Damage caused by the use of inappropriate disinfectants or the use of too high concentrations is not covered by the warranty.
8. The warranty will not be recognised if the defective mat has been previously repaired by the Customer.
9. The claimed goods are delivered at the Customer's expense.
10. In the event of an unjustified claim, the cost of shipping the goods both ways is borne by the Customer.